



100(u) Nozzle Soap Aria_4-laser, 14-color (6b-3r-3v-2uv)

Cytometer:	FACSAriaII	User:	Administrator
Cytometer Name:	FACSAriaII	Institution:	N/A
Serial Number:	1	Software:	BD FACSDiva 8.0.2
Input Device:	Manual	Date:	9/22/2017 1:37:15 PM
Sheath Pressure:	20.00		
Nozzle Size:	100		
Window Extension:	3.00		


Blue Laser
(488nm)
FSC

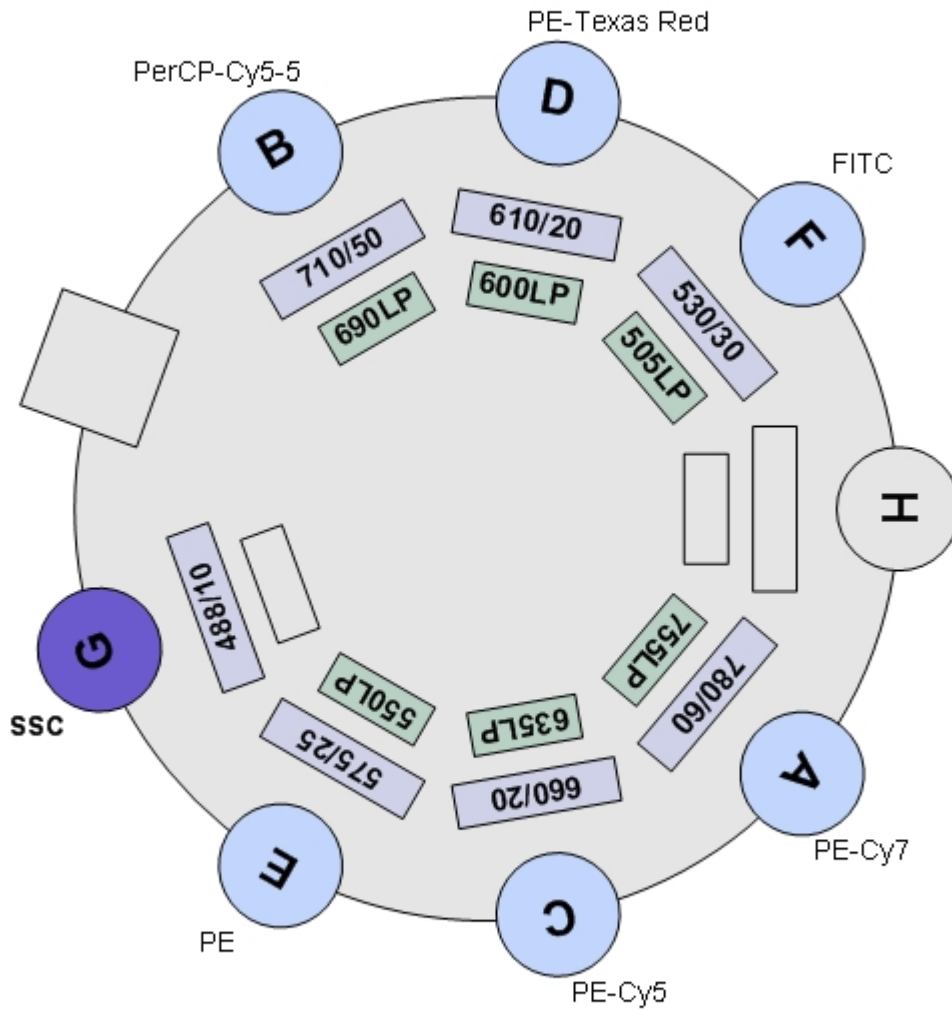


Red Laser
(640nm)

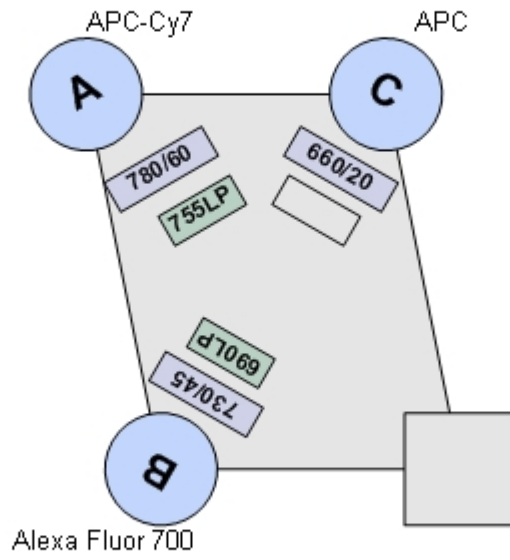

Violet Laser
(405nm)

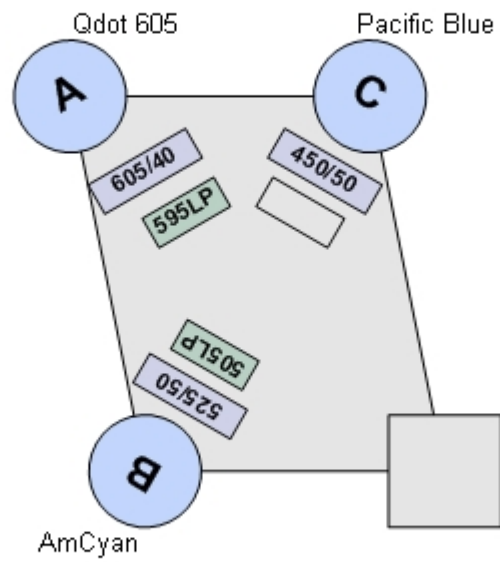

UV Laser
(355nm)

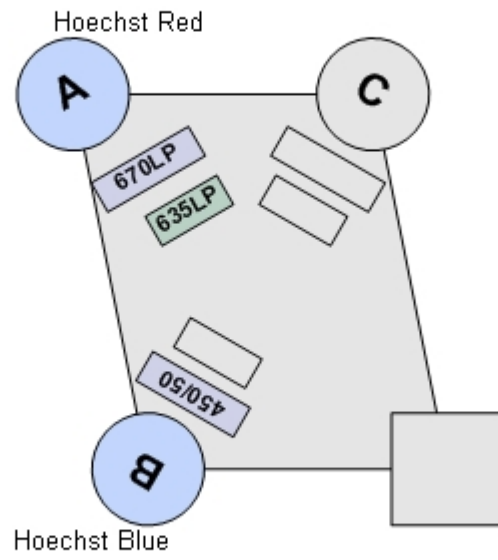

Comments: