



Fortessa5Laser16Color(5b-3r-6v-2yg) config

Cytometer:	LSRFortessa	User:	BDSERVICE
Cytometer Name:	LSRFortessa	Institution:	N/A
Serial Number:	H649225B4091	Software:	BD FACSDiva 8.0.2
Input Device:	HTS	Date:	2/14/2020 1:32:53 PM
Window Extension:	10.00		


Blue Laser
(488nm)
FSC

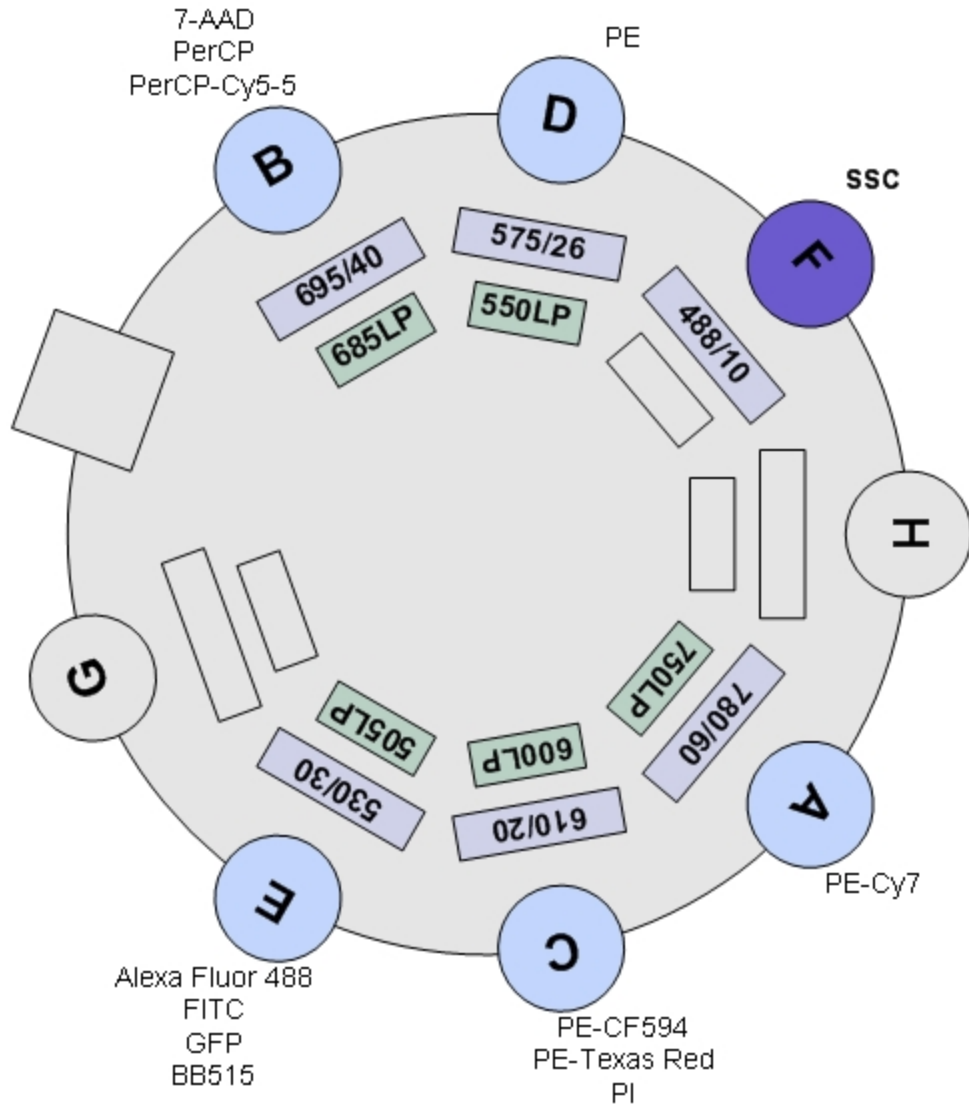


Red Laser
(640nm)

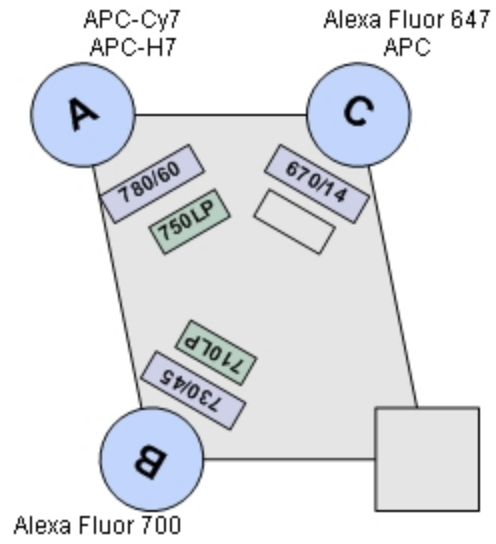

Violet Laser
(405nm)

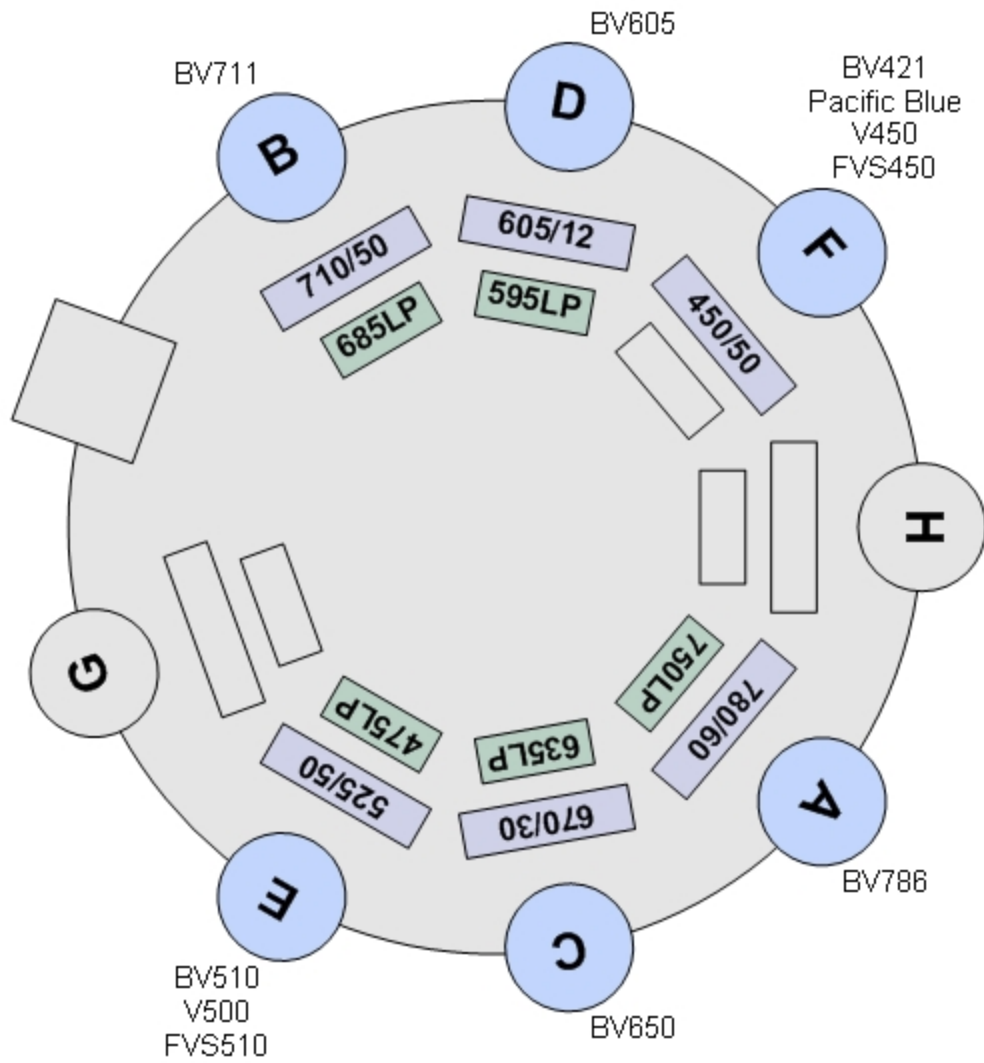

561 Yellow-Green Laser
(561nm)

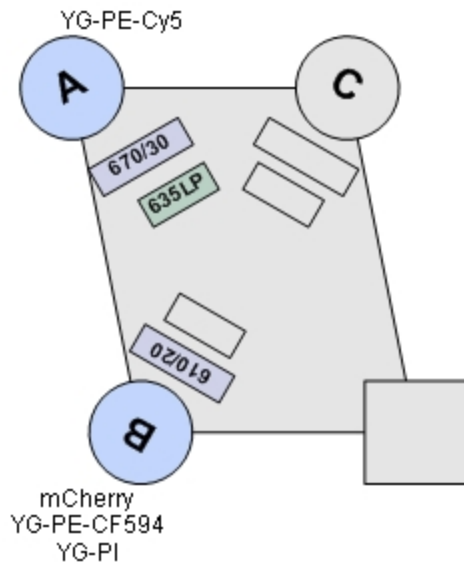

Comments: